


UniTip/UniTip HR Catheters procedure

Manual cleaning and disinfection

Cleaning




Immediately after application, rinse the catheter with warm (MAX 40°C) tap water for at least 1 minute.

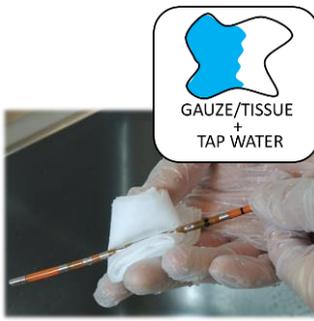

Carefully wipe the catheter with a soft gauze or tissue soaked in tap water.



If the catheter has a lumen, rinse it at least three consecutive times with a 10 ml syringe filled with cleaning solution.

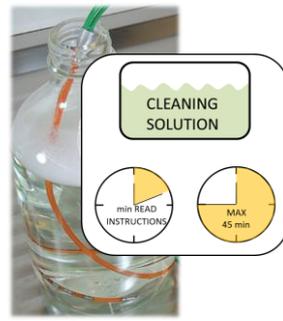

Immerse the catheter in cleaning solution for the minimal time period recommended by the manufacturer, but no longer than 45 minutes.



If the catheter has a lumen, rinse it at least three consecutive times with a 10 ml syringe filled with cleaning solution.



Wash the catheter with distilled water.



If the catheter has a lumen, rinse it at least three consecutive times with a 10 ml syringe filled with distilled water.




Carefully wipe the catheter dry with a soft gauze or tissue.

Disinfection



If the catheter has a lumen, rinse it at least three consecutive times with a 10 ml syringe filled with disinfection solution.

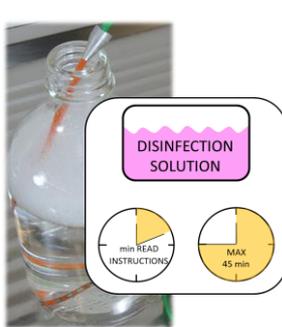


Immerse the catheter in disinfection solution for the minimal time period recommended by the manufacturer, but no longer than 45 minutes.




If the catheter has a lumen, rinse it at least three consecutive times with a 10 ml syringe filled with disinfection solution.



Wash the catheter with distilled sterile water.

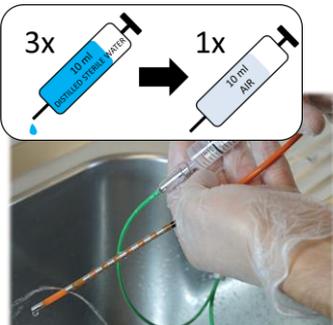

If the catheter has a lumen, rinse it at least three consecutive times with a 10 ml syringe filled with distilled sterile water. Force out any residual disinfection solution with a 10 ml syringe filled with air.

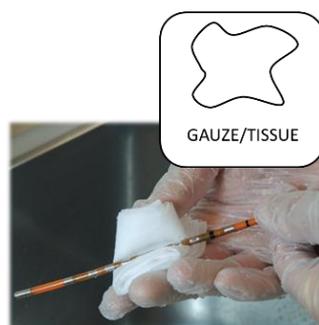

Carefully wipe the catheter dry with a soft gauze or tissue.



Wipe the connector with a soft gauze or tissue, lightly soaked in 70% cleaning alcohol.



Wipe the bottom and cover of the catheter blister with a soft gauze or tissue, soaked in 70% cleaning alcohol.



Store the catheter back into its original storage box (blister).

*If required,
continue with
sterilization...*

UNISENSOR

CUSTOMIZED SENSOR SOLUTIONS
www.unisensor.ch




Unisensor AG
Bahnstrasse 12
CH-8544 Attikon
+41 (0)52 337 37 01
info@unisensor.ch




Unisensor USA Inc.
Pease International Tradeport
112 Corporate Drive, Unit 12
Portsmouth, NH. 03801
+1 (603) 570-2675
inc.info@unisensor.ch

Attention: The IFU is authoritative for a correct reprocessing. This document is not part of the device's labelling. The latest version of this document is available on our website. Please check it with the appropriate frequency to be kept informed on the latest updates.

BEFORE USING THE CATHETER

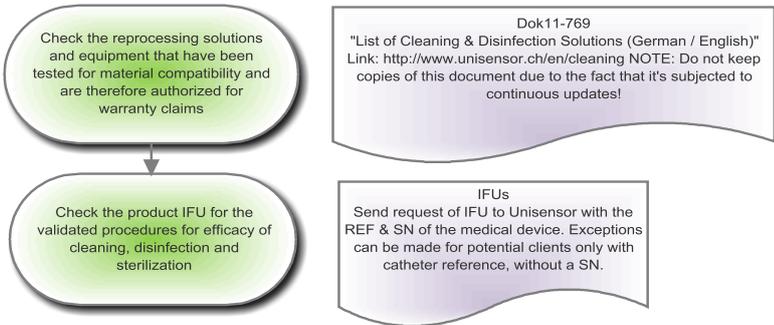

AFTER USING THE CATHETER

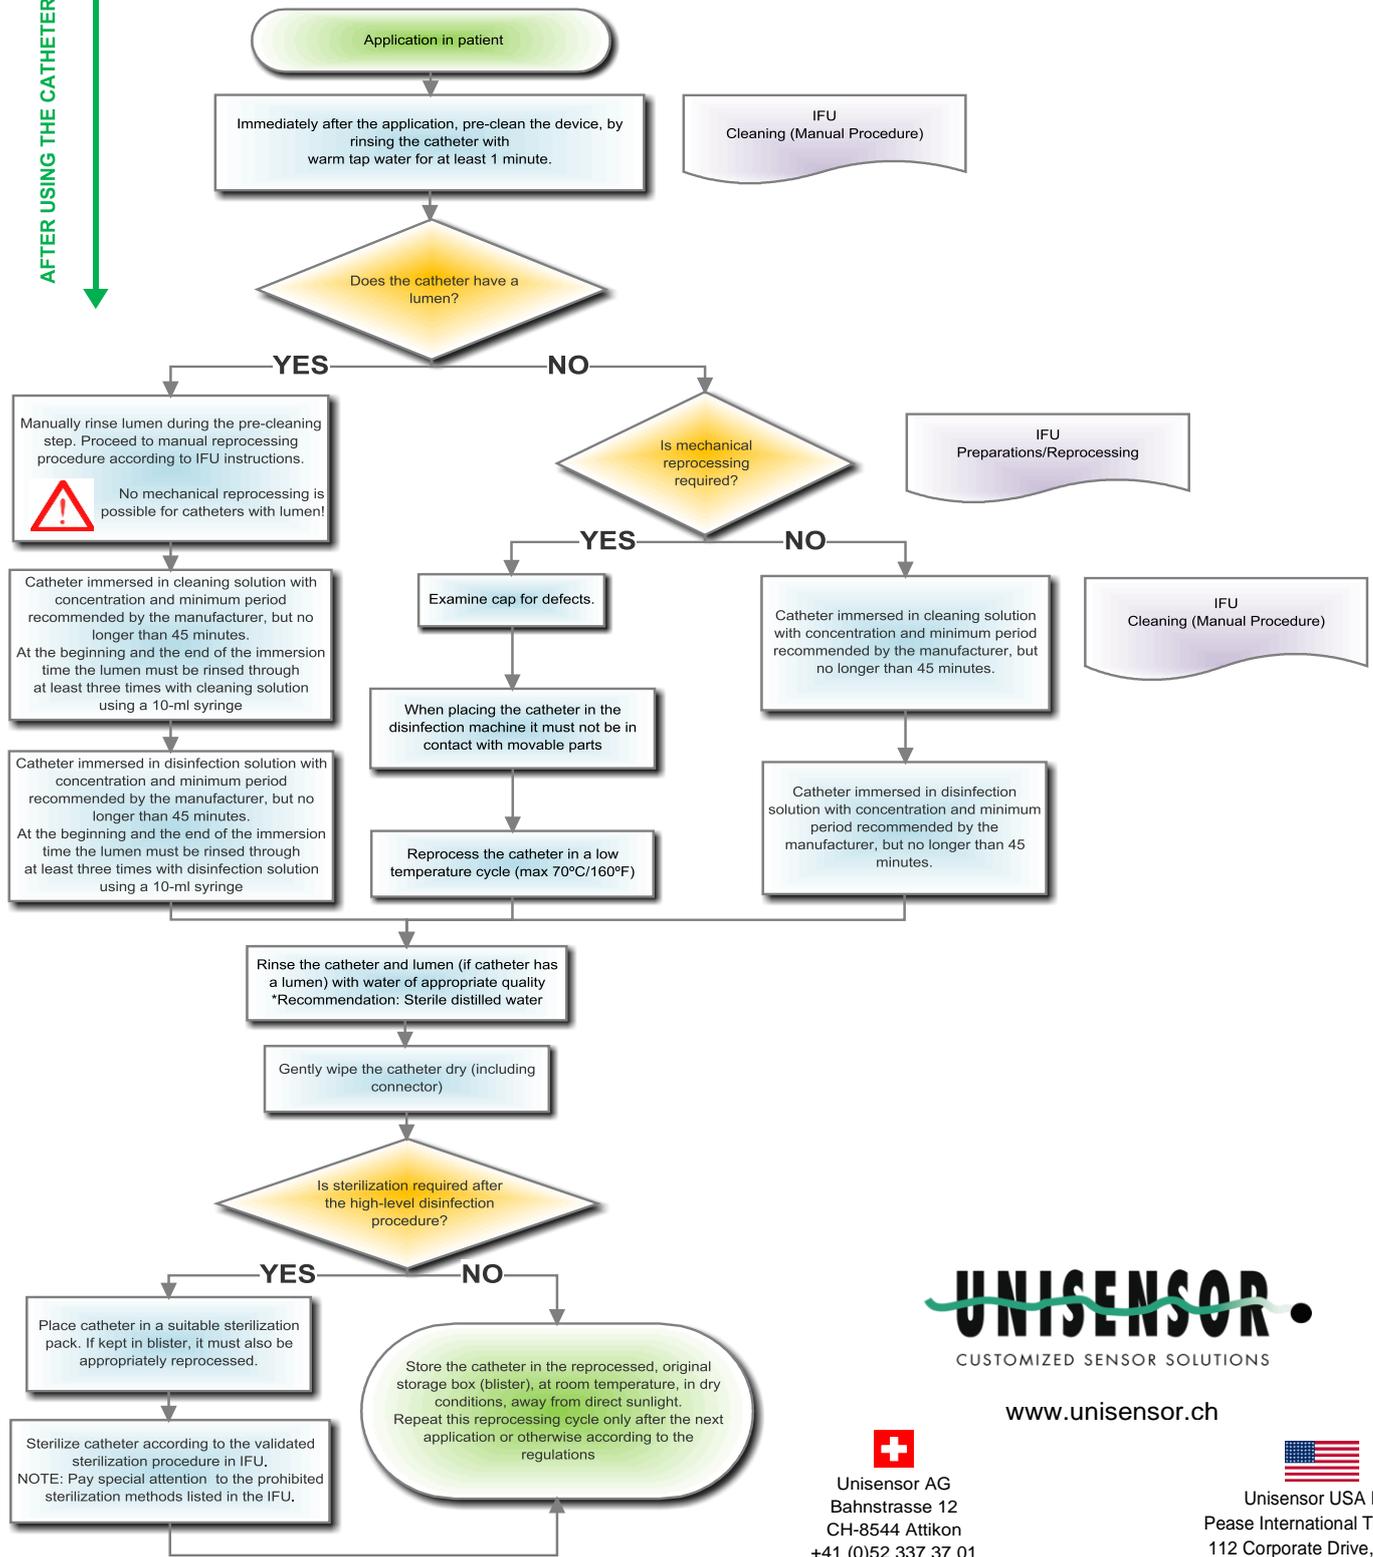

www.unisensor.ch


 Unisensor AG
 Bahnstrasse 12
 CH-8544 Attikon
 +41 (0)52 337 37 01
 info@unisensor.ch


 Unisensor USA Inc.
 Pease International Tradeport
 112 Corporate Drive, Unit 12
 Portsmouth, NH, 03801
 +1 (603) 570-2675
 inc.info@unisensor.ch